

DAC-HIT-3 is a tester that has been developed to make automatic measurements of direct current tests of appliances such as high voltage rotating machines and stator coils. The measurement voltage is output between DC 0-10kV, and after selecting polarization index (PI) mode or leakage index (LI) mode, measurement is conducted automatically for the designated duration at the configured voltage. In addition, using the memory function, data can be stored at each time, and data can be checked by using the MEM keys in front of the tester.


Furthermore, GP-IB interface that allows easy integration of automatic test systems is equipped, so can be used in insulation diagnostic systems.

Application: Direct current tests of high voltage rotating machines and stator coils.



Application:	Direct current tests of high voltage rotating machines and stator coils.		
Features:	Maximum output voltage Polarization index (PI) and leakage index (LI) are automatically measured GB-IB included suitable for optimization		
Specification			
	Output Voltage	DC 0-10000V	negative polarity
	Measuring Range:		
	Absorption Current	1x10 ⁻¹⁰ - 1x10 ⁻³ A	
	Insulation Resistance	1M ohm-9999G ohm	
		200nA Range	0-200nA (Maximum 9999 G ohms)
		2uA Range	0-2uA (Maximum 999.9G ohm)
		20uA Range	0-20uA (Maximum 99.99 G ohms)
		200uA range	0-200uA (Maximum 9999M ohm)
		2mA Range	0-2mA (Maximum 999.9M ohm)
	Resolution:	Absorption current 0.1nA (200nA Range)	
		Insulation Resistance	0.1M (2mA Range)
	Measuring Accuracy:	Current	200nA - 20uA ± 10% ± 1digit FS
			200uA - 2mA ± 5% ± 1digit FS
		Voltage	± 5% ± 1digit FS
	Interface:	GP-IB	
	Analog Output:	Range F.S +10V	
	AC Input:	AC90 - 250V 50 / 60Hz	
	Size and Weight:	W430 * H200 * D380(mm) 12kg	
	Accessories:	1. Measuring Cable (5M)	1
		2. AC Power Code	1
		3. Grounding Cable (5M)	1
		4. Accessory Bag	1

Front Panel

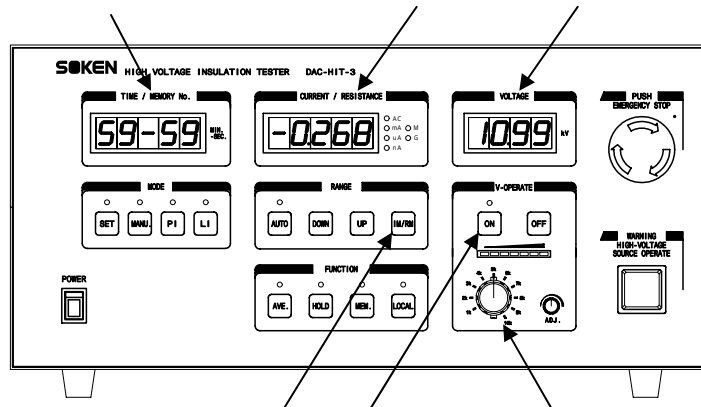

Measurement time, Memory No.
Test voltage
Test Voltage Applying Key

Current and Resistance
Current/Resistance switch key
DC Voltage Change Switch

PI (polarization index) test : Measurement for 10 minutes at designated voltage

Data memory points: 24 points

Memory data intervals: 10-second intervals from 10 seconds to 1 minute, 30-second intervals from 1 minute to 10 minutes

PI = value at 1 minute after applying voltage / value at 10 minutes after applying voltage

LI (leakage index) test : After PI test (10 minutes), leakage current is measured for 10 minutes in discharging condition.

Data memory points: 48 points (including 24 points in PI test)

Memory data intervals: 10-second intervals from 10 seconds to 1 minute, 30-second intervals from 1 minute to 10 minutes, 10-second intervals from 10 minutes to 11 minutes, 30-second intervals from 11 minutes to 20 minutes

LI = value at 10 minutes after applying voltage / value at 10 minutes after starting discharge

Connection diagram

